



Standard Specification for Use of Bar Codes on Specimen Tubes in the Clinical Laboratory¹

This standard is issued under the fixed designation E 1466; the number immediately following the designation indicates the year of original adoption or, in the case of revision, the year of last revision. A number in parentheses indicates the year of last reapproval. A superscript epsilon (ϵ) indicates an editorial change since the last revision or reapproval.

1. Scope

1.1 This specification specifies the way bar coded sample identification labels are applied to clinical specimen containers. It documents the form, placement, and content of bar code labels on specimen tubes that are used on clinical laboratory analyzers. It enables Laboratory Information System vendors to produce reliable bar coded symbols that are readable by any complying clinical laboratory analyzer vendor.

1.2 This specification is intended to apply to all clinical settings where specimens are collected from patients for examination or analysis in health care laboratory operations. It is complementary to, and extends, the Health Industry Business Communication Council (HIBCC). The document covers requirements that include the symbology, print quality measurement (wavelength of light), module width, symbol size, placement and orientation of the label, and data form and content.

1.3 The values stated in SI units are to be regarded as the standard. The values given in parentheses are provided for information only.

2. Referenced Documents

2.1 ANSI Standard:

X3.182-1990 Bar Code Print Quality Guidelines²

2.2 Other Documents:

USS-39 Uniform Symbology Specification-39³

USS-128 Uniform Symbology Specification-128³

Provider Applications Standard⁴

Guideline for the Uniform Labeling of Blood and Blood Components⁵

3. Terminology

3.1 The terminology found in X3.182-1990 shall be used where applicable.

¹ This specification is under the jurisdiction of ASTM Committee E-31 on Healthcare Informatics and is the direct responsibility of Subcommittee E31.13 on Clinical Laboratory Systems.

Current edition approved March 15, 1992. Published May 1992.

² Available from American National Standards Institute, 11 West 42nd Street, 13th Floor, New York, NY 10036.

³ Available from Automatic Identification Manufacturers, 634 Alpha Drive, Pittsburgh, PA 15238-2802.

⁴ Available from Health Industry Business Communication Council, 5110 N. 40th Street, Suite 120, Phoenix, AZ 85018.

⁵ Available from American Blood Commission, 1600 Wilson Blvd., Suite 905, Arlington, VA 22209.

4. Significance and Use

4.1 Bar code label printers and readers have been provided to accompany laboratory instruments and clinical laboratory information systems with increasing frequency in recent years. In other areas of health care, bar code technology has been successfully used to track radiographs, patient paper charts, supply requisitions, and administrative documents. In the clinical laboratory, use of the printing and reading equipment for bar codes to effectively track requests for services, specimens, and laboratory work has been impeded by the lack of common conventions. This specification provides for the use of bar codes in the management of laboratory specimens.

4.2 This specification should be used by manufacturers and vendors who configure either instruments or information handling systems for the clinical laboratory in order to provide the capabilities described in this specification. It should be used by laboratorians to develop procurement proposals that require this specification and operating procedures which utilize, to the fullest, the noted capabilities. If both audiences conscientiously adhere to this course, the greatest benefit will be obtained within the clinical laboratory through use of conforming components. Alternative considerations in making use of this specification in developing operation procedures best suited to the specific laboratory are available.⁶

5. Requirements

5.1 Symbologies:

5.1.1 *Code 39*—Code 39 shall be the symbology for printing and reading bar coded labels applied to specimen containers. The standard check digit shall be used.

5.1.2 *Code 128*—Code 128 shall be allowed and should be encouraged as a symbology for use in the future (Code 128 includes an inherent check character). Most bar code printers should have the ability to print both Code 39 and Code 128.

5.1.3 Where not explicitly defined in this specification, Specifications USS-39 or USS-128 shall apply.

5.1.4 Future readers on laboratory analyzers should be able to decode both Code 39 and Code 128 symbologies.

5.2 Symbol Dimensions:

⁶ Tilzer, Lowell L., and Jones, R., *Archives of Pathology and Laboratory Medicine*, Vol 12, 1988, pp. 1200–1202; Neely, W., *MLO (Medical Laboratory Observer)*, March 1990, pp. 24–27; Whisler, K., *Laboratory Medicine*, Vol 21, 1990, pp. 7–11.

5.2.1 *Length*—The length of the bar code symbol shall not exceed 60 mm (2.36 in.) including the required minimum quiet zone of 5 mm (0.20 in.) at each end of the symbol (see Fig. 1).

5.2.2 *Height*—The height of the bar code symbol (see Fig. 1) on the collection tube shall not be less than 10 mm (0.40 in.).

5.3 *Data Content:*

5.3.1 The entire 43 character set for Code USS-39 may be used (A–Z, 0–9, space – . \$ / + %). The entire 43 character set supported for Code 39 shall be used for Code USS-128. Full ASCII character set shall not be used for specimen identification. Leading and trailing space characters shall not be used.

5.3.2 There shall be a minimum of three data characters in the bar code.

5.3.3 The maximum number of encoded data characters permitted shall be eleven.

NOTE 1—Numeric data may be compacted for additional content, in which case base 36 should be used. If a lower density printer is used, the maximum number of data characters depends on the number of data characters that fit in a symbol which does not exceed the 60 mm (2.36 in.) limit in length, including quiet zone.

5.3.4 For specimen identification conforming to HIBCC-PAS (Provider Application Standard), the bar code shall contain, in addition to the start/stop characters and a check character specific to the symbology, the *where/what* flag characters “CD” preceding the unique specimen identification data characters. Where label length or number of specimen identification characters is limited, or in a closed identification system, the “CD” may be deleted from the sample identification and be nonconforming to HIBCC-PAS.

5.4 *Human Readable Information:*

5.4.1 Included on the collection tube in human readable form shall be all encoded data characters except start, check character and stop codes. If a compaction routine is used, then as a minimum the compacted data in human readable form shall be printed on the label.

5.4.2 The bar coded label to be affixed to the collection tube shall include an identifier that links the sample to the patient and may also include other identifiers such as the patient name, patient identification, sample identification number, date, and priority (stat, routine, ASAP, etc.) according to standard regulatory requirements. The total size of the label may be

more than 10 by 60 mm (0.39 by 2.36 in.) to allow for human readable information to be printed.

5.5 *Bar Code Label Orientation*—The label shall be placed with the bars perpendicular to the axis of the tube (see Fig. 2). The label skew shall be less than $\pm 5^\circ$ with respect to the axis of the sample container.

5.6 *Bar Code Placement*—Instrument readers shall accommodate a bar code symbol including quiet zone placed within a zone of 0 to 62 mm (0 to 2.44 in.) from rim of sample container. The label shall be applied to the cylindrical portion of the tube below the rim, skirt, or cap of the sample container.

5.7 *Module Dimension (Narrow Element Dimension)*—The narrow element dimension of the bar code symbol shall be nominally 0.19 to 0.51 mm (0.0075 to 0.02 in.).

5.8 *Bar Code Reader Wavelength:*

5.8.1 *Wavelength of Light*—The wavelength of light used for reading bar code labels should be 630 to 990 nanometers. Future instrument readers should conform to visible light range as suggested by Specifications USS-39 and USS-128.

5.9 *Print Quality of Measurement:*

5.9.1 *Wavelength of Light*—The wavelength of light used for measuring bar code labels shall be 900 nanometers $\pm 10\%$.

5.9.2 *Measuring Aperture*—The measuring aperture shall be 0.13 mm (0.005 in.) $\pm 10\%$.

5.9.3 *Symbol Grade*—The minimum acceptable symbol grade shall be “C” as defined by ANSI X3.182-1990.

5.9.4 *Print Quality of Measurement*—Where not explicitly defined in this specification, ANSI X3.182 shall apply for aspects with regard to bar code print quality.

5.10 *Other Bar Code Symbols*—There shall be no other vertically oriented bar code symbols on the specimen container.

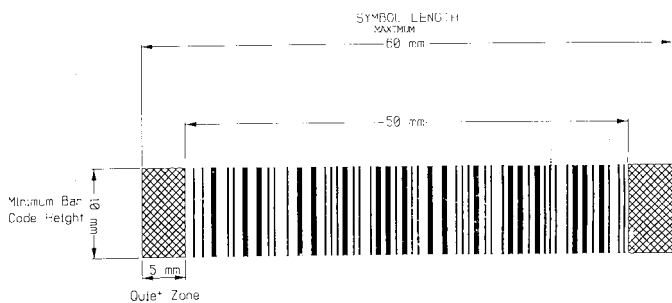


FIG. 1 Symbol Dimension

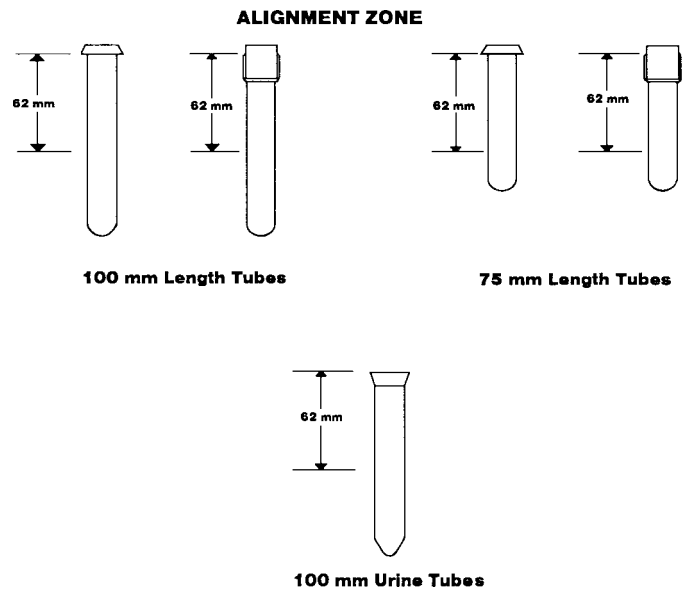


FIG. 2 Bar Code Label Placement

 **E 1466**

The American Society for Testing and Materials takes no position respecting the validity of any patent rights asserted in connection with any item mentioned in this standard. Users of this standard are expressly advised that determination of the validity of any such patent rights, and the risk of infringement of such rights, are entirely their own responsibility.

This standard is subject to revision at any time by the responsible technical committee and must be reviewed every five years and if not revised, either reapproved or withdrawn. Your comments are invited either for revision of this standard or for additional standards and should be addressed to ASTM Headquarters. Your comments will receive careful consideration at a meeting of the responsible technical committee, which you may attend. If you feel that your comments have not received a fair hearing you should make your views known to the ASTM Committee on Standards, 100 Barr Harbor Drive, West Conshohocken, PA 19428.

This standard is copyrighted by ASTM, 100 Barr Harbor Drive, West Conshohocken, PA 19428-2959, United States. Individual reprints (single or multiple copies) of this standard may be obtained by contacting ASTM at the above address or at 610-832-9585 (phone), 610-832-9555 (fax), or service@astm.org (e-mail); or through the ASTM website (<http://www.astm.org>).